

QFR 3.0

User Manual



Medis Medical Imaging Systems bv
Schuttersveld 9, 2316 XG Leiden, the Netherlands



<https://www.medisimaging.com>

On the Medis website, select “Products” and then the applicable product group. The user documentation can be found on that page.

A PDF reader is required to access the user documentation. If a PDF reader is not installed on the system, you can download the free Adobe reader. Visit the Adobe website at <https://get.adobe.com/reader/> and click “Download Adobe Reader” to download the PDF reader.

Medis Medical Imaging

Schuttersveld 9
2316 XG Leiden
The Netherlands

P +31 71 522 32 44

E support@medisimaging.com

Medis Medical Imaging Inc

9360 Falls of Neuse Road, Suite 103
Raleigh, NC 27615-2484
USA

P +1 (919) 278 7888

E support@medisimaging.com

Medis Medical Imaging Japan

Kabutocho 1st Heiwa Bldg. 3F 5-1
Nihonbashi Kabutocho, Chuo-ku, 103-0026
Tokyo, Japan

P +81(0)3 6778 2589

E support@medisimaging.com

Legal Notices

Copyright Notice

© 2016-2024 Medis Medical Imaging Systems bv. All rights reserved.

This manual is copyrighted and is protected by worldwide copyright laws and treaty provisions. No part of this manual may be copied, reproduced, modified, published or distributed in any form or by any means, for any purpose, without prior written permission of Medis Medical Imaging Systems bv. Permission is granted to freely print unmodified copies of this document as a whole, provided that copies are not made or distributed for profit or commercial advantage.

Trademark Acknowledgments

QFR is a registered trademark of QFR Solutions bv.

DICOM is the registered trademark of the National Electrical Manufacturers Association for its standards publications relating to digital communications of medical information.

Microsoft and Windows are either registered trademarks or trademarks of Microsoft Corporation in the United States and/or other countries.

All other brand, product, and company names mentioned in this document are trademarks or registered trademarks of their respective owners.

Patents

QFR is based on patented protected technology. Patents are registered in Europe under numbers NL2012459, NL2016787, NL20222109, NL20226137, EP3457945, EP3660858 and EP4231914. Patents are registered in the United States under numbers US 10,740,961, US 11,216,944 and US 11,741,602. Patents pending in Japan.

Regulatory Information

Intended Use

QFR is a medical software device intended to be used for the visualization of X-ray angiographic images. Further, QFR is intended to be used for performing calculations in X-ray angiographic images of coronary vessel segments. The calculations are based on the contours that are automatically detected, in the images of coronary vessel segments, by the software and subsequently presented to the user for review and manual editing.

QFR provides 3D models of coronary vessel segments based on contours which are automatically detected in two angiographic views of the vessel. From these, accurate anatomical quantifications are calculated of one or more lesions in the analyzed vessel segment. Further, the device determines the functional significance of individual and consecutive multiple lesions in coronary vessel segments.

In summary, QFR provides:

- Cine loop and 2D review,
- Dimensions of the cardiovascular vessels, and lesions,
- Quantitative results of coronary vessel segments based on a 3D reconstructed model,
- Quantification of the pressure drop in coronary vessels.

The analysis results obtained with QFR are intended for use by cardiologists and radiologists:

- To support the clinical decision-making process with respect to the diagnosis and possible treatment options for the coronary vessels,
- To support the evaluation of interventions or drug therapy applied for conditions of the coronary vessels.

Indications for Use

QFR is indicated for use in clinical settings where validated and reproducible results are needed to quantitatively assess X-ray angiographic images of the blood vessels, for use on individual patients with cardiovascular disease.

The QFR measurements can be applied to intermediate coronary lesions in individual patients with stable angina. The QFR measurement has not been evaluated and therefore should not be applied to non-coronary arteries, in paediatric patients, and cardiac patients with the following conditions:

- Tachycardia with frequency above 100 bpm,
- Systolic aortic resting blood pressure below 75 mm Hg,
- Atrial fibrillation.

The QFR measurement have not been evaluated and therefore should not be used in the following lesions or vessel types:

- Culprit lesions in Acute Coronary Syndrome,
- Bifurcation lesions with 1,1,1 Medina classification,
- Ostial lesions in main stem or right coronary artery,
- Distal left main lesions in combination with a proximal circumflex lesion,
- Bypass grafts,
- Grafted coronary arteries,
- Myocardial bridging.

When the quantified results provided by QFR are used in a clinical setting on X-ray images of an individual patient, they can be used to support the clinical decision-making process for the diagnosis of the patient or the evaluation of the treatment applied. In this case, the results are explicitly not to be regarded as the sole, irrefutable basis for clinical diagnosis, and they are only intended for use by the responsible clinicians.

Limitations

QFR has the following known (technical) limitations.

Restrictions on X-ray angiographic images used for QFR measurements:

- The two 2D angiographic images used for the 3D vessel reconstruction need to be taken with at least 25° difference in viewing angle.

QFR measurements cannot be performed accurately under the following conditions:

- Too much overlap of other vessels with the lesion or areas just around the lesion in the target vessel in one or both angiographic acquisitions,
- Too much foreshortening of the target coronary artery in one or both angiographic acquisitions.
- When no nitroglycerin has been administered either systemic or intracoronary,
- In vessels with retrograde fillings.

Rationale and Disclaimers



QFR must be used by cardiologists, trained technicians or trained nurses who are qualified to perform cardiac analysis. If the analysis results are used to reach a diagnosis or to guide treatment, the results must be interpreted by a qualified medical professional.




In clinical practice QFR should not be used for purposes other than those described in the sections Intended Use and Indications for Use.



Users must have sufficient proficiency in the language of the user manual, read the user manual, and become familiar with QFR to be able to obtain reliable analysis results.

European Regulations

| | |
|---|---|
|  0476 | Medis QFR XA complies with the requirements of the Dutch Medical Devices Decree (Besluit Medische Hulpmiddelen, Staatsblad 2022/190) and the European Medical Devices Regulation 2017/745. Medis QFR XA has been filed with KIWA CERMET ITALIA S.P.A. (0476). |
|---|---|

Conventions Used

The following conventions are used throughout this manual to indicate mouse and keyboard actions and to refer to elements in the user interface.

Mouse

| | |
|----------------|--|
| Click | Press and release the primary mouse button. If you are left-handed, you may have set the right mouse button as your primary mouse button. |
| Click and drag | Press and hold the primary mouse button. Drag the mouse to perform a function. Release the primary mouse button. If you are left-handed, you may have set the right mouse button as your primary mouse button. |
| Right-click | Press and release the secondary mouse button. If you are left-handed, you may have set the left mouse button as your secondary mouse button. |
| Middle-click | Press and release the wheel button or the middle mouse button. If you have a two-button mouse, press and release the left and the right mouse button simultaneously. |
| Double-click | Press and release the primary mouse button twice. |
| Wheel | Rotate the mouse scroll wheel. |

Keyboard

| | |
|-------------|--|
| Shift+click | Press and hold down the Shift key on your keyboard while you click a button or object. |
| Ctrl+K | Press and hold down the Ctrl key on your keyboard while you press K, then release both keys. |

Symbols Used



Tip: Provides helpful information or an alternative working method.



Note: Brings additional information to your attention.



Caution: Tells you to be careful when performing a task.



Warning: Warns you for a potentially dangerous situation in the image representation or analysis, which may lead to incorrect results. You are advised to follow the instructions to avoid this.

Table of Contents

| | |
|---|-----------|
| Introduction | 10 |
| 1 About QFR | 10 |
| 2 Quick Start..... | 11 |
| 3 System Requirements..... | 12 |
| 3.1 QFR Server Machine | 12 |
| 3.2 QFR Client Machines | 13 |
| 4 Support | 14 |
| Getting Started..... | 15 |
| 5 Startup..... | 15 |
| 6 Workspace | 17 |
| Working with QFR..... | 18 |
| 7 Image Acquisition..... | 18 |
| 7.1 Requirements for Image Acquisitions | 18 |
| 7.2 Acquisition Guidelines | 18 |
| 8 Select Patient / Study..... | 20 |
| 8.1 Getting the X-Ray Image Acquisitions | 20 |
| 8.2 Query and Retrieve..... | 20 |
| 8.3 Studies List | 21 |
| 9 Viewing | 24 |
| 9.1 Image Viewports | 24 |
| 9.2 Mouse Mode | 24 |
| 9.3 Mouse Actions | 25 |
| 10 Performing a QFR Analysis..... | 26 |
| 10.1 Vessel Selection | 26 |
| 10.2 Contours | 31 |
| 10.3 Results | 34 |
| 11 Review..... | 42 |
| 11.1 Show Report..... | 43 |

| | | |
|------|----------------------------------|----|
| 11.2 | Edit Analysis..... | 44 |
| 11.3 | Start New Analysis..... | 44 |
| 12 | Close Study | 45 |
| 13 | Log Off..... | 46 |
| | Reference..... | 47 |
| 14 | Description of QFR Results | 47 |

1 About QFR

QFR is a medical software device intended to be used for the visualization and analysis of X-ray Angiography (XA) images. It provides intuitive user workflows for loading, reviewing, and manipulating XA images in 2D, and provides tools for doing easy and quick measurements in XA images.

QFR supports the 3D analysis of anatomical and functional severity of lesions in coronary arteries from XA images. A 3D vessel model is reconstructed from the 2D contours of two angiographic projections with angles $\geq 25^\circ$ apart, that were acquired by monoplane or biplane XA systems. End-diastolic image frames will be used as input for the analysis, where the vessel lumen is well filled with contrast. The start and end positions and the contours of the target vessel segment are automatically detected. The 3D vessel model is then used to calculate the QFR value, being the mean pressure at the outlet of the vessel model divided by the mean pressure at the inlet. This calculation is based on an automatically detected patient-specific volumetric flow rate, and an automatically detected reference diameter that takes side branches into account.

2 Quick Start

After a successful installation, configuration, and post install test, you can load DICOM X-Ray Angiographic (XA) images into the QFR application and perform a QFR analysis.

- Open a browser window and enter the QFR server address. Log on to QFR. If needed, enter your Windows user account credentials.
- From the Studies page, find the study you want to analyze. If needed, query and retrieve the study from the PACS. Double click on the study or select the “start new QFR analysis” icon to load all XA series and start a QFR analysis.
- On entering the Vessel Selection step, QFR will automatically classify the coronary vessels that are visible and analyzable in each XA series. Select two series that provide a view on the vessel you want to analyze. QFR will automatically detect the end diastolic (ED) phases of the heart cycle, and select the frame that corresponds to the optimal ED phase that can be used for the analysis. If available, the ECG signal will be displayed. Verify the ED frame selection, change the frame selection if needed, and click Next to proceed to the next step in the analysis.
- On entering the Contours step, QFR will automatically detect the start and end points of the target vessel, detect the pathline, and detect the contours. Verify the start and end points, and make corrections if needed by dragging the points to the proper location. Verify the pathline and make corrections if needed by dragging the pathline to the proper location. Verify the contours and make corrections if needed by dragging the contours to the proper location. Click Next to proceed to the next step in the analysis.
- On entering the Results step, QFR will automatically detect the lesions in the target vessel and calculate the QFR result. In the Physiology tab, you can verify the Delta QFR, Residual QFR, and Diameter Stenosis % values. In the Morphology tab, you can verify the Minimal Lumen Diameter, the Reference Diameter and the Lesion Length. Verify the detected lesions and make corrections to the lesion markers if needed by dragging them to the proper location. Click Finish to complete the QFR analysis.
- On entering the Review step, the report will be created and automatically saved to the QFR data repository, and automatically exported to the PACS (if configured). Click the Show Report button to open the report. Click the Edit Analysis button to go back into the Results step of the QFR analysis where you can make changes to the analysis. Click the Start New Analysis button to start a new QFR analysis, for example on a different vessel type.

3 System Requirements

QFR should be installed on a Windows computer that acts as the server machine (preferably but not necessarily a Windows Server system). After the server is installed and configured, it can be accessed from a web browser from machines that have network access to the server. The following paragraphs list the system requirements for the server and the client machines.

3.1 QFR Server Machine

For the server machine, hardware and operating system requirements are defined.

3.1.1 Hardware

The following minimal hardware requirements are defined for the QFR server:

- Processor: 64 bit, 8 cores
- Memory: 16 GB RAM
- Hard drive: Minimal 10 GB free disk space during operation
- Network connection: Network speed \geq 100Mbps and latency \leq 50 ms

Notes:

- The hardware must be compliant with the operating system.
- Hard drive: On the QFR server machine the XA image data will be received (from X-Ray acquisition system or PACS) and cached to ensure that images are quickly available for review and/or editing. The hard drive should be big enough to keep Windows, the QFR software, and approximately 6 months of QFR study data. The actual amount of disk space needed for the image data is dependent on the number of QFR studies that you perform. For performance reasons, it is not recommend to store the QFR study data on a network drive.
- Graphics card and display: The QFR server machine does not require a dedicated graphics card or display monitor.

3.1.2 Operating Systems

The following operating systems are supported to run QFR:

- Microsoft Windows Server 2022, 64-bit
- Microsoft Windows Server 2019, 64-bit
- Microsoft Windows 10, 64-bit
- Microsoft Windows 11, 64-bit

3.2 QFR Client Machines

For the client machine, hardware and web browser requirements are defined.

3.2.1 Hardware

The following **minimal** hardware requirements are defined for the QFR clients:

- Processor: 64 bit, 4 cores
- Memory: 8 GB RAM
- Network connection: Network speed \geq 100Mbps and latency \leq 50 ms

Notes:

- The hardware must be compliant with the operating system.
- On the QFR client machines, no applications will be installed and no data will be cached.
- Graphics card and display: The QFR application will work correctly when running in a web browser on a screen with the size of a desktop computer. A screen resolution of 1.3 Megapixels or higher (e.g. at least 1280 x 1024 pixels for a display ratio 4:3, at least 1600 x 900 pixels for display ratio 16:9) is advised. Scaling and zooming may affect the display of QFR.

3.2.2 Web Browsers

The following web browsers are supported to run QFR:

- Microsoft Edge, version 116 or newer
- Google Chrome, version 116 or newer

4 Support

Medis is committed to offering high-quality products and services. If you have questions about the software or if you would like to make suggestions for improvements in the software or in the documentation, please contact the Medis helpdesk.

If you contact the Medis helpdesk by e-mail, mention “QFR 3.0.26.6” in the subject field.

Europe, Africa, Australia and Asia (excluding Japan)

Medis Medical Imaging

E-mail: support@medisimaging.com

Telephone: +31 71 522 32 44 (working days 9.00-17.00 CET)

North and South America

Medis Medical Imaging Inc

E-mail: support@medisimaging.com

Telephone: +1 919 278 7888 (working days 9.00-17.00 EST)

Japan

Medis Medical Imaging Japan

E-mail: support@medisimaging.com

Telephone: +81(0)3 6778 2589 (working days 9.00-17.00 JST)


Getting Started

5 Startup

The QFR application must be accessed from a web browser, by visiting or browsing to the QFR server address. The server address is dependent on the installation and configuration for your organization (e.g. <https://qfr.myorganization.com>).

- 💡 QFR is running on a server machine in your organization network, it does not make use of a QFR server that runs in the cloud or internet.
- 💡 You can add bookmark in your browser to save the QFR server address, and quickly open the QFR application.
- 💡 Press 'F11' on your keyboard to run QFR full screen.

The logon screen of the QFR application will be presented.

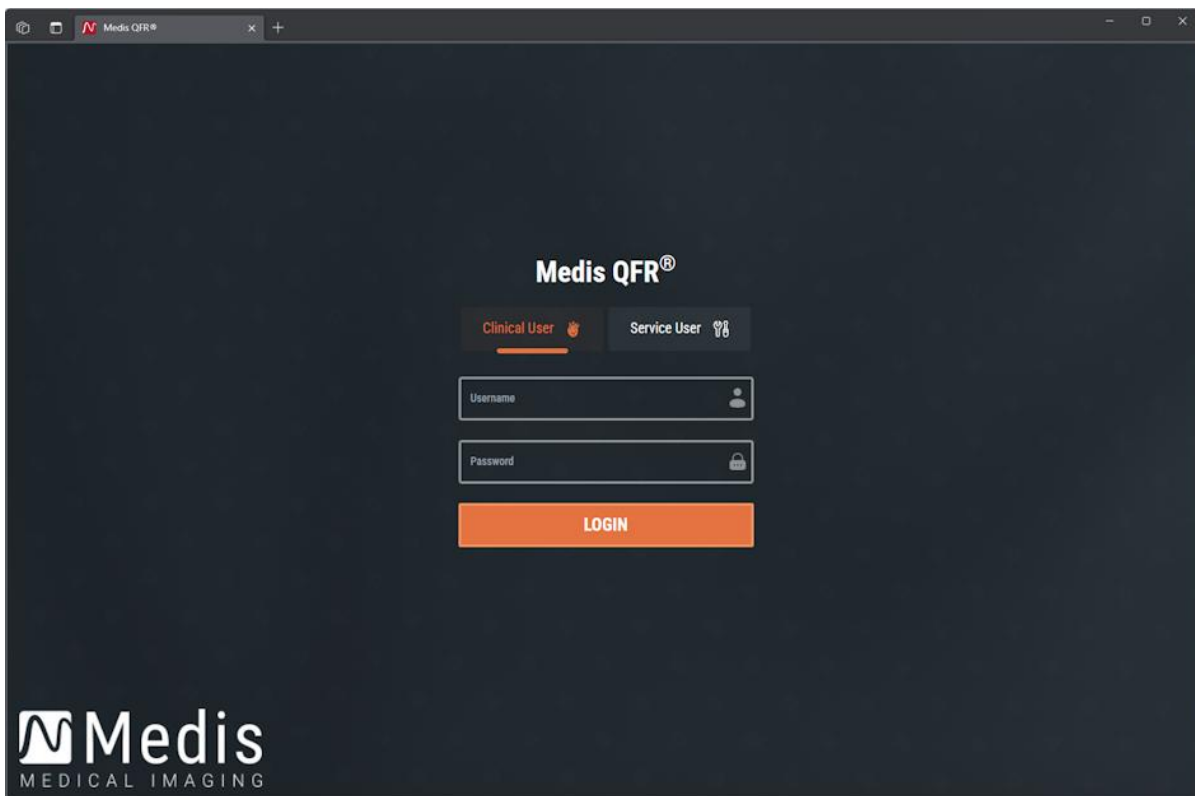

To logon to QFR:

- Select the Clinical User tab
- Enter the Windows username and password for your organization to log on to QFR.



Depending on the configuration for your organization, the Username and Password edit fields may or may not be visible.



You may not be authorized to work with QFR yet. In this case, contact your system administrator to request access to QFR.




After the initial configuration of QFR, the “Service User” option to logon to QFR is only available for Medis Installation and Support team members.

6 Workspace

After you have successfully logged on to QFR, the application workspace will be presented to you.

The default view will show you the **Studies** page, with an overview of all studies with X-Ray Angiography (XA) images and their QFR analyses.

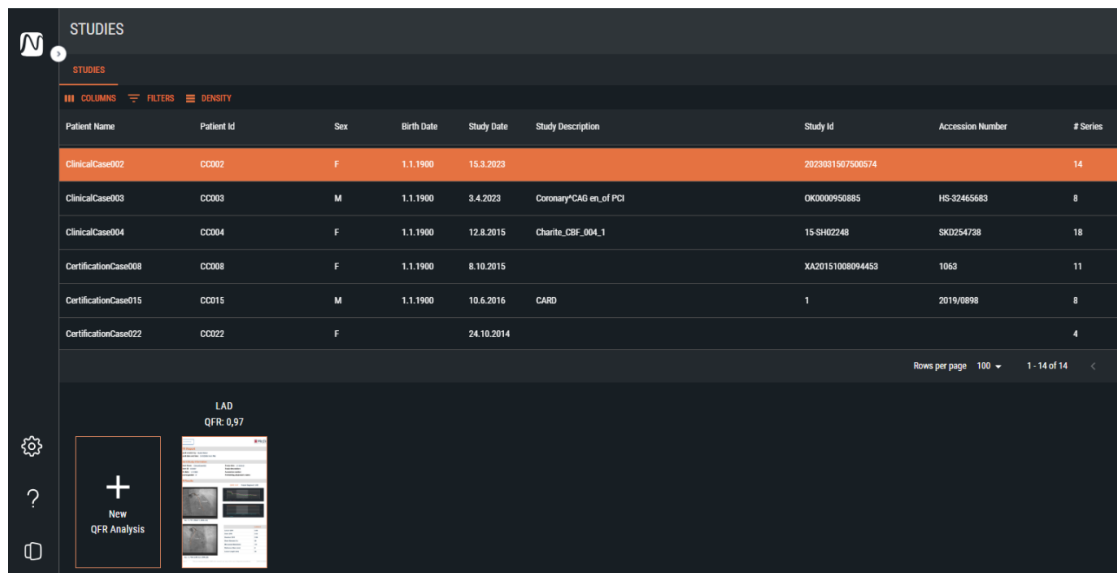

| Patient Name | Patient Id | Sex | Birth Date | Study Date | Study Description | Study Id | Accession Number | # Series |
|----------------------|------------|-----|------------|------------|------------------------|-------------------|------------------|----------|
| ClinicalCase002 | CC002 | F | 1.1.1900 | 15.3.2023 | | 2023031507500574 | | 14 |
| ClinicalCase003 | CC003 | M | 1.1.1900 | 3.4.2023 | CoronaryCAG en. of PCI | OK0000950885 | HS-32465683 | 8 |
| ClinicalCase004 | CC004 | F | 1.1.1900 | 12.8.2015 | Charite_CBF_004_1 | 15-SH02248 | SK0254738 | 18 |
| CertificationCase008 | CC008 | F | 1.1.1900 | 8.10.2015 | | XAX20151008094453 | 1063 | 11 |
| CertificationCase015 | CC015 | M | 1.1.1900 | 10.6.2016 | CARD | 1 | 2019/0898 | 8 |
| CertificationCase022 | CC022 | F | | 24.10.2014 | | | | 4 |

Rows per page: 100 | 1 - 14 of 14





LAD
QFR: 0.97

New QFR Analysis



QFR will only load studies with XA series. In case your study has image data from other modalities (such as MR or CT) they will not be visible in the list.

In the side bar on the left the following functionalities are available:

-  to return to the main screen (study browser or QFR analysis)
-  to open the Settings screen, which includes:
 - general application configuration,
 - configuration of users and roles (only accessible for users with Administrator role),
 - configuration of DICOM connections (only accessible for users with Administrator role),
 - the 'post install test'.
-  to open the Help screen, which includes:
 - information how to contact the Medis support team,
 - information about the QFR application,
 - the QFR user documentation,
 - information about the available QFR licenses,
 - the QFR audit trail.
-  to log off from QFR.

7 Image Acquisition

7.1 Requirements for Image Acquisitions

DICOM XA image monoplane or biplane acquisitions can be used as input for the QFR analysis if they comply to the following criteria:

- The images are expected to be in grayscale (not color),
- The images must have square pixels (pixel aspect ratio 1:1),
- The images are accompanied by isocenter calibration data,
- The images are acquired at fixed angulations (no rotational angiography),
- The images are expected to have at least 5 image frames. (This is to filter out single frame and other very short acquisitions such as balloon interventions, and wires without contrast. An acquisition suitable for the QFR analysis will include approximately 3 full heart cycles.)



DICOM XA images that do not comply to the above criteria will automatically be excluded from the QFR analysis, and they will not be visible as thumbnails in the Vessel Selection step.

7.2 Acquisition Guidelines

The QFR analysis is based on a 3D vessel reconstruction. To create a successful reconstruction, two XA acquisitions of the target vessel will be required, acquired from two different angles. The two acquisitions must have an angle difference of $\geq 25^\circ$ (optimally between 35° and 50°). Also, the projections should be as perpendicular as possible to the target vessel (not parallel).

Recommendations for the angiographic procedure:

- Prior to the first angiographic acquisition to be used for QFR analysis, inject intracoronary nitroglycerin.
- Use a frame rate of at least 12.5 frames per second.
- Use a 4F catheter size or larger.
5F or larger is recommended to support a brisk injection of the contrast.
- Make sure that the entire catheter is filled with contrast before the injection.
Prevent premature contrast leakage.
- Use brisk, continuous and fast contrast injections.
Aim for 3 full cardiac cycles (i.e. fully opacified target vessel).
- Minimize overlap of target segments (especially at the lesions).
- Avoid foreshortening of the target vessel.
- Prior to the acquisition, inject some contrast to check potential severe overlap and/or severe foreshortening. If any, rotate or angulate 5° more.

- Avoid moving the table early after injection (during acquisition).
- Ask the patient to hold their breath if possible (during acquisition).
- Make sure that the entire target vessel is visible in both image projections.

Recommendations for the default first and second projections of a target vessel (all angles based on monoplane acquisitions):

| Vessel/Bifurcation | 1st View | 2nd View |
|--------------------|-----------------|-----------------|
| LM + LAD/LCX | RAO 20 , CAU 25 | AP , CAU 10 |
| LAD/Diag | AP , CRA 45 | RAO 35 , CRA 20 |
| LCX/OM | LAO 10 ,CAU 25 | RAO 25 , CAU 25 |
| Prox + Mid RCA | LAO 45 , CAU 0 | AP , CAU 0 |
| PLA/PDA | LAO 45 , CAU 0 | LAO 30 , CAU 30 |



QFR does not require image acquisitions of patients in hyperemic state as input for the analysis.

8 Select Patient / Study

From the Studies page, find the study you want to analyze. If needed, query and retrieve the study from the PACS. Double click on the study or select the “start new QFR analysis” icon to load all XA series and start a QFR analysis.

8.1 Getting the X-Ray Image Acquisitions

There are two ways to make the X-Ray image acquisitions available for QFR. Both scenarios will have to be configured by your system administrator and/or PACS administrator:

- The acquisitions can be ‘pushed’ directly from the X-Ray acquisition system to the QFR server. The ‘push’ can either be triggered automatically or manually, depending on your clinical practice and the functionality supported by your X-Ray acquisition system.
In this workflow, no user interaction is needed in the QFR application to receive the images. After the images have been received by QFR, they will immediately be available in the studies page as input for the analysis.
- The acquisitions can be ‘queried and retrieved’ from your PACS system to the QFR server.
In this workflow, from the QFR application, you query for a specific patient study in the PACS archive. Afterwards, you can retrieve a copy onto the QFR server. After all images of the study have been received by QFR, they will be available in the studies page as input for the analysis.

How to query and retrieve a study is described in the next section.

8.2 Query and Retrieve

To query and retrieve studies from the PACS:

- Select the tab **Query / Retrieve from PACS**
- If multiple PACS systems are configured, select the PACS that holds the study that you want to retrieve in the drop down box **From PACS**.
- Specify one or multiple of the query parameters:
 - Patient Name
 - Patient ID
 - Study ID
 - Accession Number
 - Study Date (default: last 7 days)
- Select **Query** to search for studies that match with the query parameters. The results of the search will be displayed in the study list.
- Select the study from the list that you want to retrieve to QFR.
- Select **Retrieve** to retrieve all information from the selected study to QFR.

The status of the retrieve will be presented in the first column of the query result list.



Make sure that you provide sufficient query fields to limit the search results from the PACS. Some PACS systems will support wild card characters ('?' to match any single character, and '*' to match any multiple characters).



Some, but not all, PACS systems will also report the 'Number of images in the study' as part of the query result. If this information is available to QFR, it will be presented in the second column of the query result list.

8.3 Studies List

After the X-Ray acquisitions have been pushed or retrieved to QFR, they will be presented in the Studies list. The studies list shows columns with the relevant patient and study information.


| Patient Name | Patient Id | Sex | Birth Date | Study Date | Study Description | Study Id |
|----------------------|------------|-----|------------|------------|--|-----------|
| CertificationCase015 | CC015 | M | 1/1/1900 | 6/10/2016 | CARD | 1 |
| CertificationCase022 | CC022 | F | | 10/24/2014 | | |
| TrainingCase002 | TC002 | M | 1/1/1900 | 7/1/2015 | Coronary*Diagnostic Coronary Catheterization | 2015/0913 |
| TrainingCase006 | TC006 | | 1/1/1900 | 11/11/1111 | Cardiac | 301 |
| TrainingCase007 | TC007 | M | | 6/14/2017 | | |
| TrainingCase012 | TC012 | M | 1/1/1900 | 2/9/2011 | Coronary*Diagnostic Coronary Catheterization | 1 |
| TrainingCase026 | TC026 | M | | 6/14/2017 | | |

To show or hide columns from the studies list:

- Select **COLUMNS** and enable or disable the columns that you want to show or hide

If there are many studies available, it can become harder to find the study that you want to analyze. To help you find the study of interest, QFR provides filter and sort options.

To filter the entries in the studies list:

- Select  to activate the filter control.
- Select the column that you want to use in your filter.
- Enter the filter value, e.g. patient name “john” to only show the patients that have the characters “john” in their full name.

You can filter on text values for patient name, patient ID, sex, study description, study ID, accession number and number of series in the study.

You can filter on date values or date ranges for the patient birthdate and study date.


To sort the entries in the studies list:

- Hover your mouse on one of the columns in the header of the study list, to show the sort icon (arrow up).



- Click on the arrow icon to sort the entries in the study list ascending (arrow up).
- Click on the arrow icon again to sort the entries in the study list descending (arrow down).



The options to show or hide columns, and filter and sort items in the list are also available from the menu  in each column of the header.

If you select a study from the studies list, the QFR analysis list will show the analyses that have been performed earlier for this particular study. The analysis can be reopened, reviewed, and edited.

The screenshot shows a software interface with a table of studies and two RCA analysis thumbnails below it. The table has columns for Patient Name, Patient Id, Sex, Birth Date, Study Date, and Study Description. The first row is highlighted in orange. Below the table, there are two thumbnails for RCA analysis, each with a QFR score of 0.83 and 0.89 respectively. A 'New QFR Analysis' button is visible on the left side of the analysis area.

| Patient Name | Patient Id | Sex | Birth Date | Study Date | Study Description |
|----------------------|------------|-----|------------|------------|------------------------|
| TrainingCase007 | TC007 | M | | 6/14/2017 | |
| ClinicalCase003 | CC003 | M | 1/1/1900 | 4/3/2023 | Coronary*CAG en_of PCI |
| CertificationCase015 | CC015 | M | 1/1/1900 | 6/10/2016 | CARD |
| ClinicalCase001 | CC001 | M | 1/1/1900 | 1/16/2023 | CARD March 2017 |
| CertificationCase008 | CC008 | F | 1/1/1900 | 10/8/2015 | |
| ClinicalCase002 | CC002 | F | 1/1/1900 | 3/15/2023 | |
| ClinicalCase004 | CC004 | F | 1/1/1900 | 8/12/2015 | |

The QFR analysis are sorted from the latest analysis (on the left) to the oldest analysis (on the right). Hover your mouse on top of the QFR analyses to see the name of the analyst, and the date and time the QFR analysis was created.

To load a study and start QFR analysis:

- Select a study entry in the Studies list
- Double click on the study entry
- Or, right click on a study entry, and select “New QFR Analysis”
- Or, click on the icon “New QFR Analysis” from the analysis list

To load an existing QFR analysis:

- Select a study entry in the Studies list
- Select a QFR analysis in the analysis list
- Or, right click on the QFR analysis icon, and select “Load QFR Analysis”

You can also remove a study or a QFR analysis from the study list or analysis list.

To delete a study:

- Select a study entry in the Studies list
- Right-click on the study entry, and select “Delete Study”

To delete an analysis:

- Select an analysis entry in the Analysis list
- Right-click on the analysis entry, and select “Delete QFR analysis”

9 Viewing

This chapter describes the functionality for viewing images that is available in the QFR analysis steps.

9.1 Image Viewports

The QFR analysis workflow steps have two image viewports that display the XA image data. Each viewport has a viewport control toolbar. Some viewports have textual overlays that can also be interactive. An example of a viewport is given in the following image:



9.2 Mouse Mode

The behavior of the **primary mouse button** (the left button for a right-handed mouse) depends on the mouse mode: panning, zooming, or window width and level. The mouse mode can be set by using the buttons in the viewport control toolbar. The toolbar button that is highlighted indicates the active mouse mode.

To activate a mouse mode:

- Select the appropriate toolbar button:



for panning



for zooming



for window width and window level



Although each viewport has its own viewport toolbar, the mouse mode for the different viewports are synchronized; changing the mode in one viewport will also change it in the other viewport.

The behavior of the **secondary mouse button** (the right mouse button for a right-handed mouse) is always connected to the window width and window level functionality.

The behavior of the **middle mouse button** is always connected to the zooming functionality.

The mouse **scroll wheel** can be used to scroll through the individual frames of the cine. Scroll up to activate higher frame numbers, and scroll down to activate lower frame numbers.

9.3 Mouse Actions

The image viewports also have mouse actions. The mouse actions can be activated using the buttons in the viewport control toolbar.

To activate a mouse action:

- Select the appropriate toolbar button:



to **reset the viewport** to the default values for zoom, pan, and window width and window level.

Resetting the viewport will also reactivate the analysis frame.



to **hide the overlay** with the graphics that are displayed on top of the image.

The graphics overlay will be hidden while the button is pressed, and will be displayed again when the button is released.

10 Performing a QFR Analysis

When you load a study, the QFR analysis will automatically start. QFR will guide you through three workflow steps that are required to complete the analysis. You will be asked to provide manual input, or to verify and confirm the output of the QFR algorithms.

The following workflow steps are defined:

- Vessel Selection
- Contours
- Results

In the next sections, each workflow step will be described in more detail.


10.1 Vessel Selection

1 Vessel Selection — 2 Contours — 3 Results

On entering the Vessel Selection step, QFR will automatically classify the coronary vessels that are visible and analyzable in each XA series. Select two series of the target vessel you want to analyze. QFR will automatically detect the end diastolic (ED) phases of the heart cycle, and select the frame that corresponds to the optimal ED phase that can be used for the analysis. Verify the ED frame selection, change the frame selection if needed, and click Next to proceed to the next step in the analysis.

In the Vessel Selection step of the QFR analysis, you need to select the coronary vessel that you want to analyze and select two XA series and ED image frames that have a proper view on this target vessel. The selected ED image frames will be used as the input ('analysis frames') for the QFR analysis.

In the Vessel Selection step, the screen shows the series selection controls at the top, the frame selection controls at the bottom, and the image viewports in the middle.

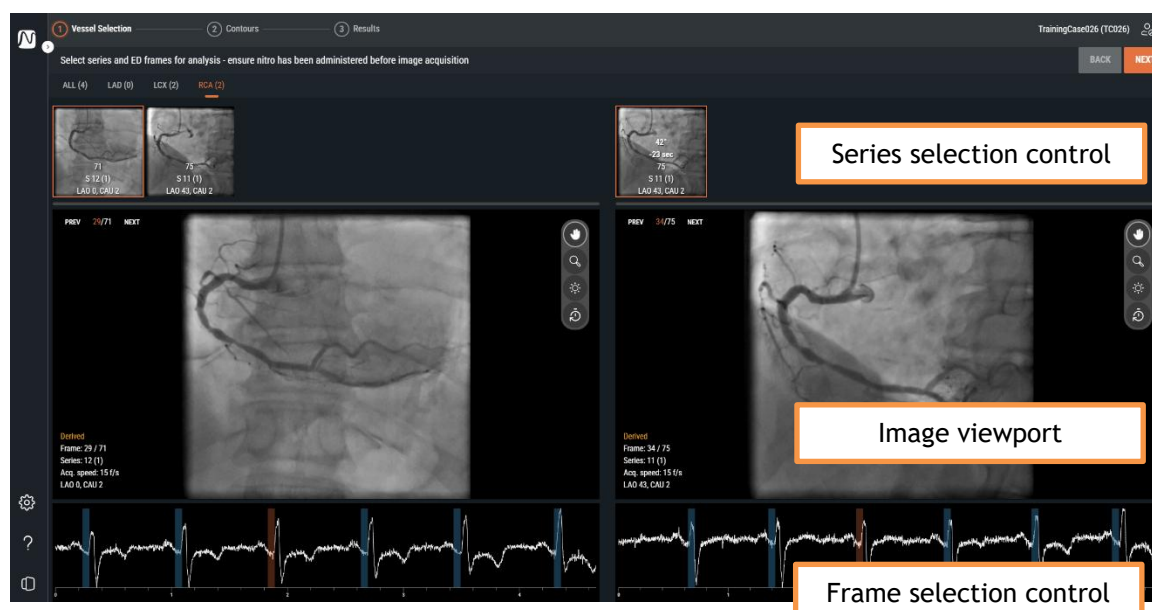

The series selection control, the image viewport and frame selection control will help you select the two XA acquisitions and ED image frames that will be the input for the QFR analysis. Both should have a proper view on the target vessel, they must be acquired at different angulations (at least 25° apart) and within a certain time frame (maximum 2 hours apart).


10.1.1 Series Selection Control

When you enter the Vessel Selection step, QFR will automatically process the XA series with an artificial intelligence (AI) algorithm to detect the most probable coronary vessel that is visible and analyzable in the image data. QFR can detect the following coronary vessels:


- Left Anterior Descending (LAD)
- Left Circumflex (LCX)
- Right Coronary Artery (RCA)

The XA series with the same vessel type are grouped together on a tab. The XA series are presented as thumbnails, with an overlay that shows the number of frames, series number, and the angulation and rotation of the gantry during the acquisition.

The ALL tab displays all XA series of the study, independent of the detected vessel type, if they are suitable as input for the QFR analysis.

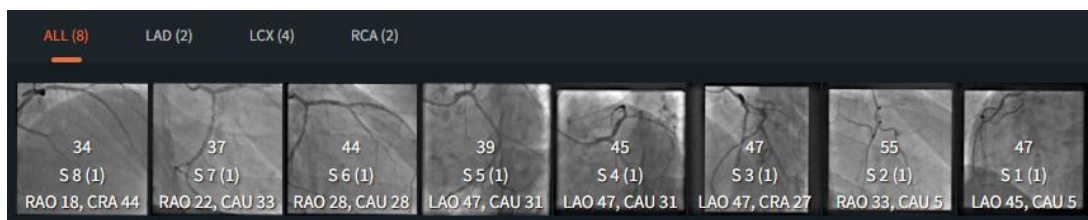

The LAD, LCX and RCA tabs will only display the XA series of the study with the corresponding image type that are suitable as input for the QFR analysis.

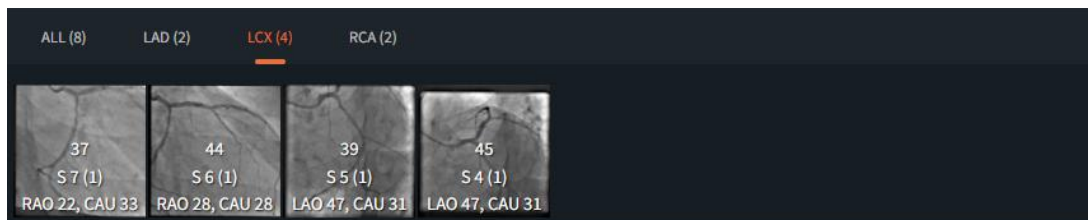



Not all XA series may be classified as LAD, LCX or RCA, for example if the algorithm is not able to detect a vessel type, or the XA image does actually not show one of the main vessel types. The ALL tab will show all XA series that are suitable as input for the analysis, independent of the automatically detected vessel type.


When you select a thumbnail in the series selection control, the corresponding XA series will be loaded in the image viewport below.

To select the two XA series as input for the QFR analysis:

- Select a vessel type tab in the left series control: All, LAD, LCX, or RCA.
- Select a series in the left series selection control. This will load the corresponding XA series in the left image viewport. The series selection control on the right will be populated with the XA series that could be a suitable matching pair; this includes only the series of the same vessel type, acquired at least 25° apart, and within 2 hour time frame.
- Select a series on the right hand selection control. This will load the corresponding XA series in the right image viewport.

The following image shows an example where two LAD series have been selected as input for the QFR analysis.

- The LAD tab is selected.
- On the left series number 4 has been selected (LAO 0, CRA 45).
- On the right series number 5 has been selected (RAO 35, CRA 20).
- Series numbers 4 and 5 have a 3D angle difference of 38°, and an acquisition time difference of 45 seconds.

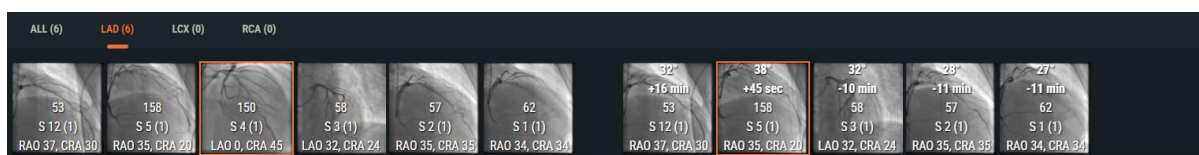

If possible, QFR will automatically select the matching XA series in the right series selection control.


- If there are only 2 series available for a vessel type, selecting one on the left side, will automatically load the other one the right side.
- If you select one series of a biplane acquisition on the left side, the other series will automatically load on the right side.

10.1.2 Frame Selection Control

After selecting the XA series, you need to select the appropriate image frames as input for the QFR analysis.



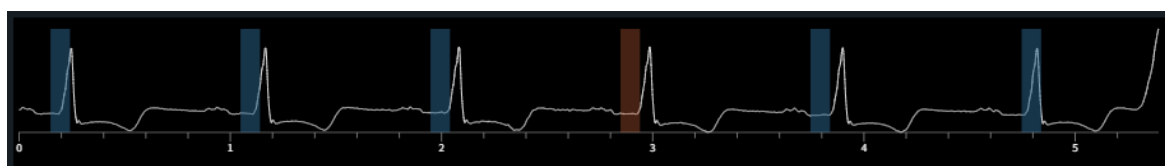

The QFR analysis should be performed on an image frame that is in the end diastolic (ED) phase of the heart cycle, where the heart is in a state of rest. QFR will automatically detect all image frames that are in an ED phase, by examining the electrocardiogram or by reviewing the image data using an AI algorithm. From all ED image frames, QFR will automatically select the one that is considered to be optimal as input for the QFR analysis, by examining the contrast filling of the vessel.


The frame selection control is shown below each image viewport. On the x-axis, time is displayed in seconds. The orange vertical bar indicates the selected image frame, visible in the corresponding image viewport. The blue bars indicate the image frames that correspond to the automatically detected ED phases. If ECG data is included with the image data, the ECG curve is shown in the frame selection control.



Verify the image frame that was automatically selected by the system is suitable to be used as input for the analysis. If needed, you can select another image frame in the ED phase of the cardiac cycle to be used as input for the QFR analysis.

To change the active image frame:

- Click in the frame selection control to select the image frame at the corresponding time point.
- Or, click and drag the mouse in the frame selection control to continuously update the active image frame.
- Or, click the frame selection controls in the angiographic viewport.
 - Click the PREV button (lower frame numbers)
 - Click the NEXT button (higher frame numbers)
- Or, use the arrow keys on your keyboard.
 - Use arrow keys left  (lower frame number) and right  (higher frame number) to change the active image frame in the **left** image viewport.
 - Use arrow keys down  (lower frame number) and up  (higher frame number) to change the active image frame in the **right** image viewport.

After you have selected two image frames suitable the QFR analysis, click  to proceed to the next workflow step of the QFR analysis.

Points of attention

- The frame for analysis must be in the ED phase of the cardiac cycle.
- The vessel and lesion(s) of interest should be clearly visible with good contrast filling and as little overlap as possible with other structures.

To verify if QFR automatically selected the proper end diastolic phase:

- The arteries are stretched as much as possible.
- For left and right coronaries arteries find the image in which the aortic valve opens and the accumulated contrast flushes into the aorta and then go backwards 2 or 3 frames backwards.


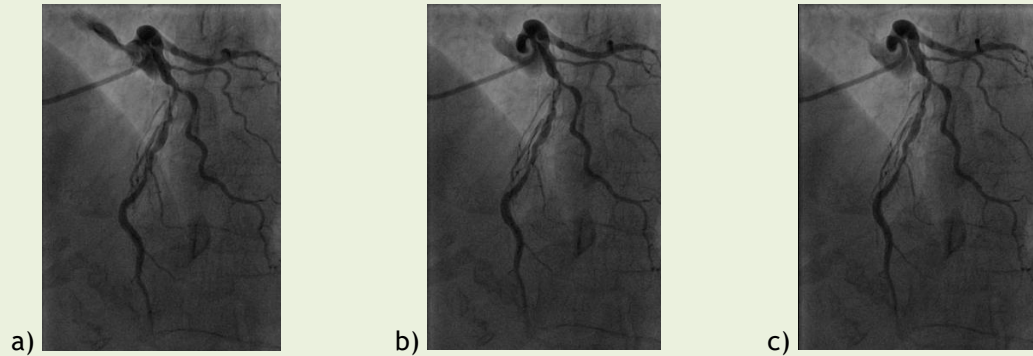


Figure a) shows the accumulated contrast flushing to the aorta, b) 1 frame earlier from frame a) and c) depicts the ED frame.

Another method to verify the end diastolic frame for left tree is when the vessel is in the most upper position of the image:



- For right coronary analysis, another way to find the ED frame is to look at moment where the angles formed by the posterior descending and posterolateral arteries widens.

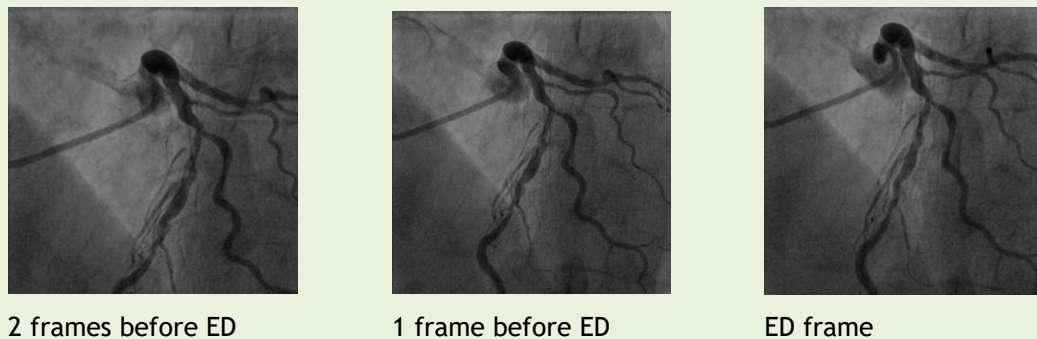

10.2 Contours

Vessel Selection — 2 Contours — 3 Results

On entering the Contours step, QFR will automatically detect the start and end points of the target vessel, detect the pathline, and detect the contours. Verify the start and end points, and make corrections if needed by dragging the points to the proper location. Verify the pathline and make corrections if needed by dragging the pathline to the proper location. Verify the contours and make corrections if needed by dragging the contours to the proper location. Click Next to proceed to the next step in the analysis.

In the Contours step of the QFR analysis, you need to verify that QFR detected the correct start and end points of the target vessel, a pathline between them, and the contours of the vessel. If needed, you can make corrections manually.

In the Contours step, the screen only shows the two image viewports.



When you enter the Contour step, QFR will automatically detect the start and end points of the target vessel that is visible and analyzable in the XA series. Afterwards, it will detect the pathline from start to end point, and the contours of the target vessel. The contours from both views will be used as input for the 3D vessel reconstruction.

If the start or end point, the pathlines, or the contours are not detected properly, you can edit them manually in the image viewports.

To edit start or end points:

- Click and drag the start (● red) and end (● blue) points to the proper location.

To edit a pathline:

It might be that an incorrect pathline is detected (e.g. when the target vessel is crossed by another vessel). In this case you can add one or more support points to guide the pathline through the segment of interest.

- Click a point on the pathline and drag it to the correct position.
This creates a support point and redetects the pathline and the contours.
- If needed add more support points or drag existing support points to better locations.



If editing is required, correct the pathline before making corrections to the contours.

To delete a pathline support point:

- Right-click on the support point to delete it.
The pathlines between the proximal and distal points and the contours are redetected automatically.

To edit a contour:


It could also be that the vessel contours are not detected correctly along the entire length of the target vessel. In this case you can add one or more support points to the contours.


- Click a point on the contour and drag it to the correct position.
This will create a contour support point and redetect the corresponding contour.
- If needed add more support points or drag them to better locations.

To delete a contour support point:

- Right-click on the contour support point.
The point is deleted, and the corresponding contour is redetected.



Use the **Hide Overlay** button  to hide all graphics and have a clear view at the image data. This will help you to verify the correct placement of the contours.

When you are confident that the start and end point, the pathline, and the contours of the target vessel have been placed correctly, click  to proceed to the next workflow step of the QFR analysis.

Points of attention

- Proximal and distal points must be placed in the same anatomical points in both views.
- The proximal point should be placed at the ostium of the target vessel.
- Avoid setting the proximal point on top of the catheter tip.
- The distal point must be placed distally in the vessel, where you normally will allocate a pressure wire.
- Verify that all the disease portions of the vessel are included in the vessel segment.
- Be sure to include all lesions and enough healthy areas in the vessel of analysis.

After checking the start and end points it is important to check the automatically generated contours as well. Therefore, pay attention to:

- Contours at the beginning and end of the pathline: the contour can be bent inwards creating a false lesion.
- Side branches.
- Overlapping vessels: this situation might cause diameter size overestimation.
- Low contrast acquisition also causes inwards bending.

Pitfalls and particularly difficult lesions

Left main artery (LM)

The LM and RCA ostiums are difficult to assess due to the guiding catheter intrusion, or the back flow of contrast agent into the aorta overlapping the ostium. Currently, the presence of an ostial LM or RCA stenosis excludes the use of QFR (is a software limitation).

Left main artery (LM) + Left anterior descendent artery (LAD)

If there are stenoses in both the LM and LAD, it is very important to place the proximal point proximal to the stenosis in the LM.

Left circumflex artery (LCX)

The LCX ostium might be difficult to assess due to the requirement of two optimal projections. In many cases only one optimal projection can be acquired.

Left main artery (LM) + the ostium of the circumflex artery (CX)

This combination cannot be analyzed in one time, due to differences in physiological flow patterns in these vessel types. For the left main analysis you need to indicate the vessel type in the software LM/LAD and for circumflex analysis you need to select LCX.

In this case it is advised to first perform an analysis of the LM in the direction of the LAD and determine if the lesion in the LM is significant or not. The lesion in the CX needs to be analyzed in a separate analysis as well. But, as stated earlier, a lesion in the ostium of the CX is very difficult to visualize in two views with more than 25° difference in angiographic view.

10.3 Results

Vessel Selection — Contours — **3 Results**


On entering the Results step, QFR will automatically detect the lesions in the target vessel and calculate the QFR result. In the Physiology tab, you can verify the Delta QFR, Residual QFR, and Diameter Stenosis % values. In the Morphology tab, you can verify the Minimal Lumen Diameter, the Reference Diameter and the Lesion Length. Verify the detected lesions and make corrections to the lesion markers if needed by dragging them to the proper location. Click Finish to complete the QFR analysis.

In the Results step of the QFR analysis, the Physiology and Morphology results will be calculated and presented on the screen. The screen shows the image viewports on tabs on the left:

- Angiogram 1
- Angiogram 2
- 3D View

and the results on tabs on the right:

- Physiology
- Morphology

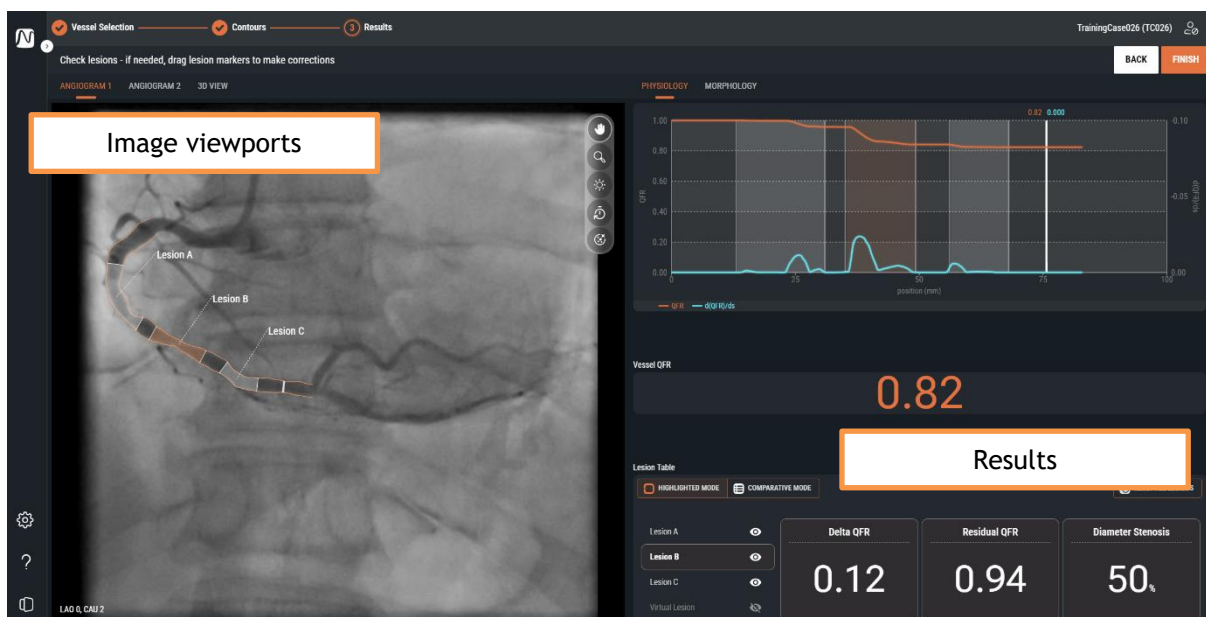

10.3.1 Image Viewports


There are two image viewports that show the angiograms, and one viewport that shows the 3D vessel reconstruction.

To switch between the different image viewports:

- Click on the tab labels “Angiogram 1”, “Angiogram 2”, or “3D View”

The **angiogram image viewports** show the angiogram with the target vessel contours and all detected lesions as graphical overlays. Each lesion is labeled with its lesion identifier. The most significant lesion (having the highest Delta QFR value) is automatically selected and highlighted. You can activate and verify the detailed parameters for each lesion.

The **3D View viewport** shows the 3D reconstruction of the target vessel. The 3D reconstruction is color coded based on the QFR values. In this view, only the lesion markers of the active lesion are visible, as well as the index marker.

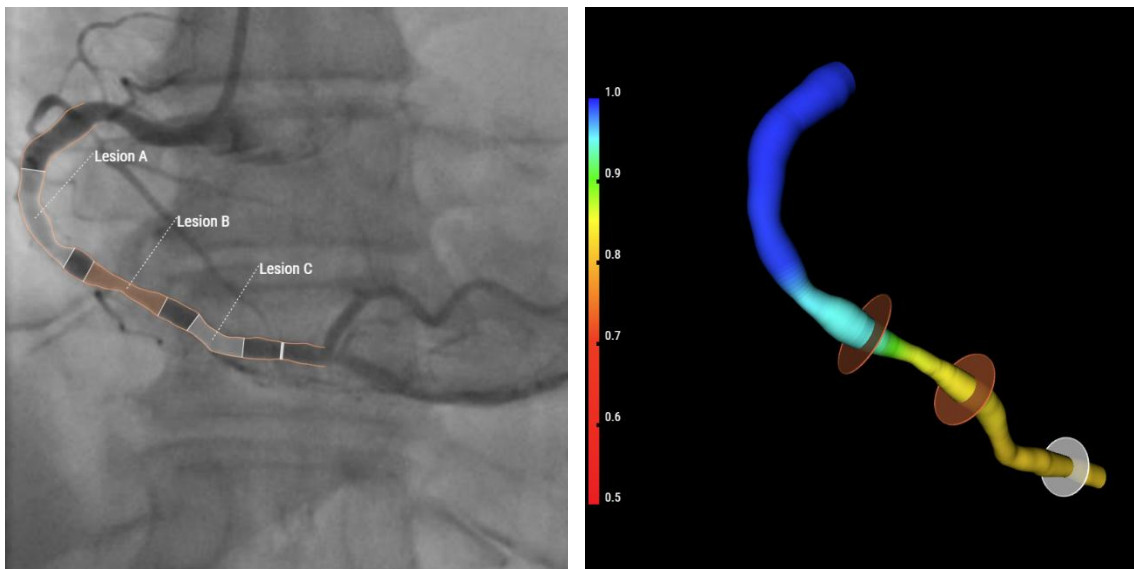

To activate the detailed lesion results in the angiogram image viewport:

- Hover your mouse on the lesion label.

This will show a text box with the detailed lesion results. By default, this includes Delta QFR, Residual QFR, Diameter Stenosis %, Minimal Lumen Diameter, Reference Diameter, and the Lesion Length.



In the QFR Settings you can configure which lesion results are presented in the text box.


10.3.2 Results

The results are presented in two tabs that are focused on the physiology results and morphology results.

To switch between the different results:

- Click on the tab labels “Physiology” or “Morphology”

In the **Physiology** tab, the QFR diagram is shown, with the curves for the QFR value and the $d(QFR)/ds$ value across the length of the target vessel:

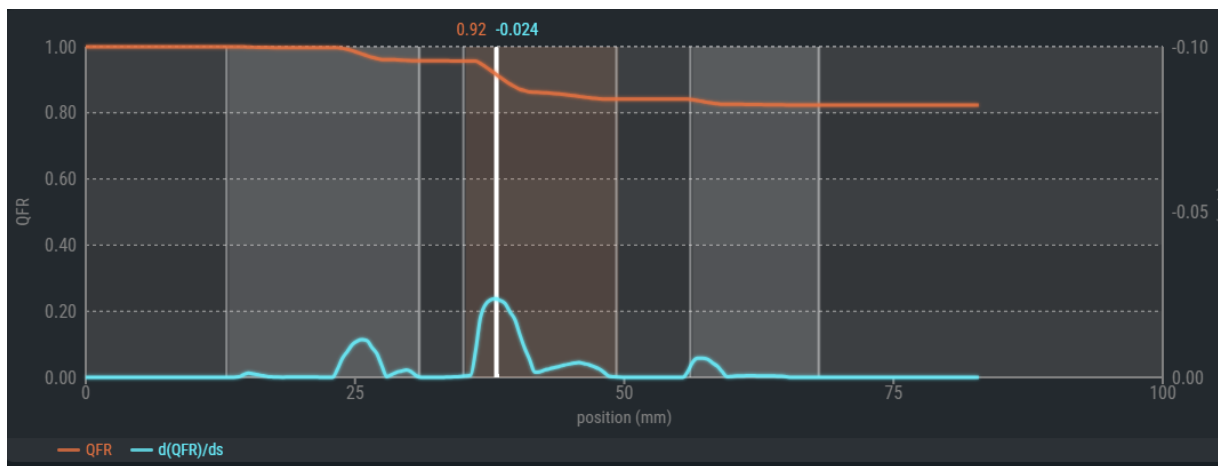

The QFR values are plotted on the left-hand y-axis. The $d(QFR)/ds$ values are plotted on the right-hand y-axis.

The QFR diagram also shows the ‘index marker’ in white. The QFR and $d(QFR)/ds$ values at the index marker are displayed at the top of the marker. You can select and drag the marker across the entire length of the target vessel.

To change the location of the index marker:

- Click on the white index marker in the QFR diagram.
- Drag the marker to the desired location.




The index marker is also visible in the Diameter diagram, the angiographic views, and the 3D view. They will all be updated when you change the position of the index marker.

Below the QFR diagram, the vessel QFR result is displayed. The vessel QFR is the simulated pressure at the end of the target vessel divided by the pressure at the start of the target vessel (see also Chapter 14).



At the bottom of the page, the lesion table with the physiological parameters is displayed.

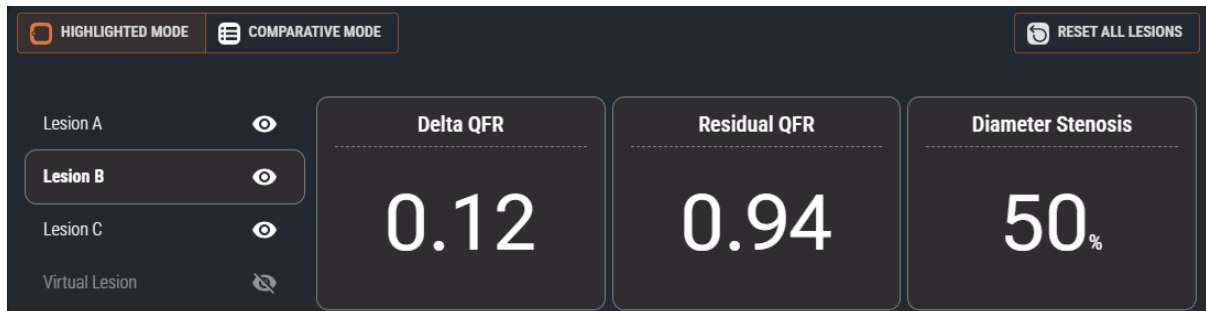

The following lesion results are displayed (see also Chapter 14):

- The **Delta QFR**: The relative change in pressure between the lesion proximal and distal marker.
- The **Residual QFR**: A predictive value of the Vessel QFR after treatment (revascularization) of the lesion.
- The **Diameter Stenosis %**. The ratio between the diameter reduction and the reference diameter.

In the **Morphology** tab the Diameter diagram is shown, with the curves for the minimal, maximal, and reference diameters.



The Diameter diagram also shows the ‘index marker’ in white. The minimal diameter and reference diameter values at the index marker are displayed at the top of the marker. You can click and drag the marker across the entire length of the target vessel.

To change the location of the index marker:

- Click on the white index marker in the Diameter diagram.
- Drag the marker to the desired location.




The index marker is also visible in the QFR diagram, the angiographic views, and the 3D view. They will all be updated when you change the position of the index marker.




If the reference diameters are outside the normal range (either very large or very small) a warning message will be displayed in the angiographic views. Make sure that the reference diameters are correct and suitable for this patient.



Below the Diameter diagram, the vessel QFR result is displayed.

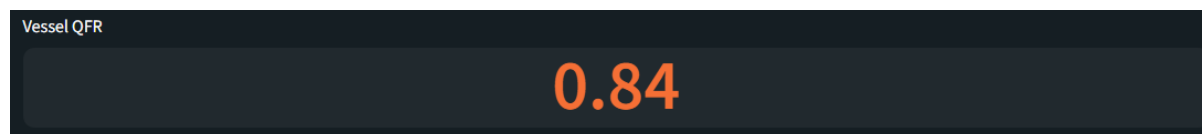

And at the bottom of the page, the lesion table with the morphological parameters is displayed.

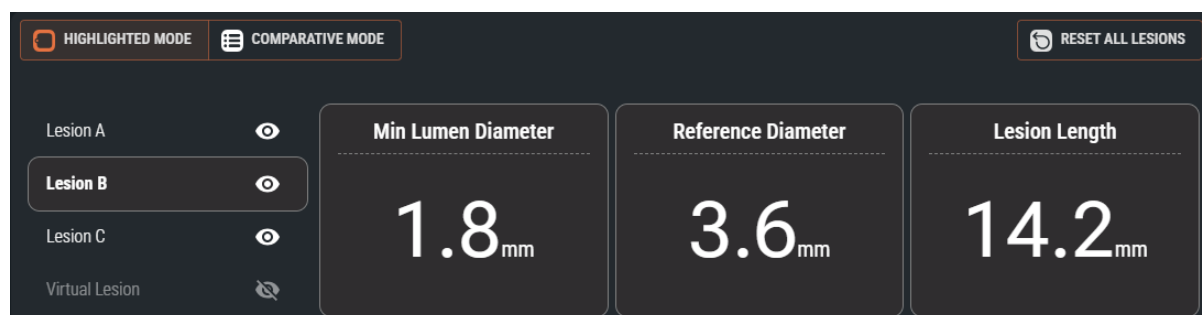

The following lesion results are displayed (see also Chapter 14):

- **Minimal lumen diameter:** The smallest lumen diameter of the lesion in mm.
- **Reference diameter:** The expected lumen diameter of a healthy vessel at the location of the minimal lumen diameter.
- **Lesion length:** The length of the lesion in mm, measured from the proximal lesion marker to the distal lesion marker, in the 3D vessel reconstruction.


10.3.3 Lesion Results

In both the Physiology and Morphology tab, the lesion results can be verified in ‘highlighted’ and ‘comparative’ mode.


To switch the lesion results tables between the different modes:

- Click on the buttons to switch to  or 

In the highlighted mode, you can only see the results of the selected lesion.

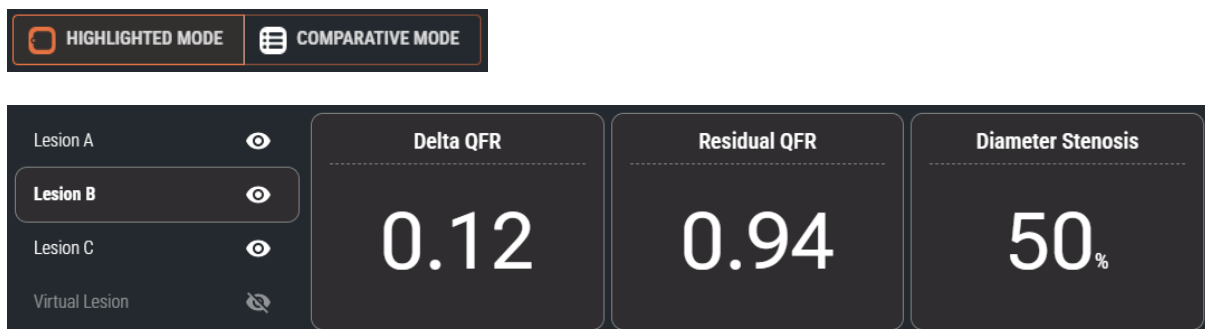

In the comparative mode, you can see the results of all lesions in one overview, to make it possible for you to compare the values against each other. The values of the selected lesion have a different font color and font size.

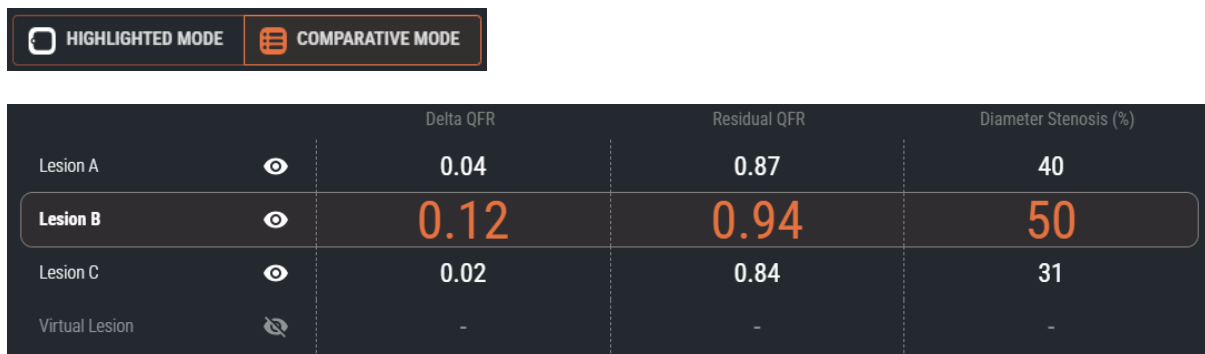



10.3.4 Editing Lesions

The lesions that have been detected by QFR can be adjusted by dragging their proximal or distal markers. You can also disable a lesion, to hide it from the overlays, diagrams and report.

To adjust the lesion markers:


- Click and drag the proximal and/or distal markers to the required positions. The markers can be dragged in the angiogram viewports, in the QFR diagram, or in the Diameter diagram. The lesion results will be updated automatically.

When a lesion is enabled, it shows the visible icon  in the lesion results table. The enabled lesion is visible on the angiogram, the diagrams, and in the report.


When the lesion is disabled, it shows the hidden icon  in the lesion results table. The disabled lesion is not visible on the angiograms, the diagrams, or in the report.

To enable or disable a lesion:

- In the lesion results table, click on the visibility icon next to the lesion label.

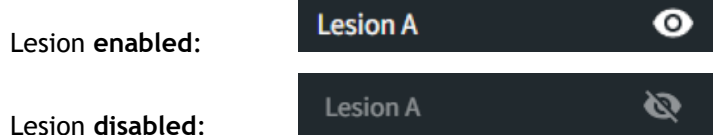



10.3.5 Complete QFR Analysis

When you are confident that the lesions have been placed correctly, click  to complete the QFR analysis.



Completing the analysis will automatically save the QFR analysis and report, and will automatically archive the QFR analysis and report on your PACS (if configured).



If you do not want to archive the QFR analysis, do not click  the QFR analysis, but close the study instead .

Points of attention

Please check that the reference diameter (red line in the diameter diagram) satisfies the following requirements:

- The reference diameter should always taper downward in the distal direction, or it should be horizontal.
- The reference diameter should follow the diameters of the healthy/normal areas.
- The reference diameter should not follow the diameters of the obstructed or aneurysmatic areas.
- The obtained reference diameter values should be realistic according to gender of the patient.



A proper reference diameter is crucial for a proper QFR calculation. The reference diameter determines the severity of the lesions along the target vessel, and the severities determine the final QFR results.

Most of the time having inaccurate contours will cause wrong reference diameters. If this occurs, go back to the Contour step and verify that the contours are defined correctly, modify them if needed. Alternatively, use another acquisition with better contour definition and less vessel overlap.

Not checking the reference diameter and correcting the contours (when necessary) can lead to wrong QFR results.

11 Review

The Review screen of the QFR analysis will show when a QFR analysis is closed, and when you reload a QFR analysis from the Studies page.

From this screen you can review the QFR analysis, including the contours, the lesions, and all physiological and morphological results. You cannot make any changes to the QFR analysis in this screen.

From the Review screen, you can also trigger the following actions:

- Show the QFR report
- Edit the QFR analysis
- Start another (new) QFR analysis on the same study.
-



The screen layout in the Review screen is exactly the same as the screen layout of the Results screen of the QFR analysis. See Chapter 10.3 and Chapter 14 for a detailed description of the available viewports and results.

In the Review screen, you cannot enable or disable the individual lesions, and not change the proximal and distal lesion markers.

11.1 Show Report

The QFR report will provide you with a one-page overview of the patient details, study details, and QFR results, including screenshots of the angiograms, the QFR diagram, and the diameter diagram. The QFR report can be downloaded in PDF format.

The screenshot displays the QFR report interface. The report is titled "QFR Report" and includes the following information:

- Report created by:** Guido Rebel
- Report date and time:** 04/12/2024 10:30 AM
- Patient Study Information:**
 - Patient Name:** TrainingCase026
 - Patient ID:** TC026
 - Birth date:**
 - Age and gender:** M
 - Study date:** 06/14/2017
 - Study description:**
 - Accession number:**
 - Performing physician's name:**
- QFR Results:**
 - QFR: 0.82**
 - Vessel Segment: RCA**

The report also includes a QFR diagram showing the vessel segment and a diameter diagram. The interface includes a "SHOW REPORT" button and a "DOWNLOAD" button.

To show the QFR report:

- Click **SHOW REPORT** to show the Report screen.





To download the QFR report in PDF format:

- From the Report screen, click the Download button **DOWNLOAD**

11.2 Edit Analysis

To make changes to the QFR analysis, for example to make a correction to the detected contours or lesions, you can edit the QFR analysis.

To edit the QFR analysis

- Click  to reactive the QFR analysis guided workflow. You will enter the Results step (the last step of the workflow).
- If needed, click  to step back to earlier steps of the QFR analysis guided workflow.
- Make all required changes to the QFR analysis, as described in sections 10.1, 10.2 and 10.3.
- Click  and/or  to close the QFR analysis and save the modified QFR analysis.






When you edit a QFR analysis and finish it, it will always be saved as a 'new' analysis and not overwrite the 'old' analysis.

11.3 Start New Analysis

You can always start a new QFR analysis from the QFR Studies page, but this can also be started from the Review screen.

To start a new QFR analysis

- Click 
- QFR will load all XA series of the active study, and start a new QFR analysis, starting at the Vessel Selection screen.
- Make all required changes to the QFR analysis, as described in sections 10.1, 10.2 and 10.3.
- Click  and  to close the QFR analysis and save the new QFR analysis.

12 Close Study

When you have completed all QFR analyses, or want to cancel an open QFR analysis, you can return to the Studies page by closing the active study.

To close the active study:

- Click Close Study The icon is a dark square containing three orange circles arranged in a triangle, with a white circle containing a diagonal slash overlaid on the bottom-right circle.






Closing the study will cancel the open QFR analysis.

13 Log Off

To end your active QFR session, you can log off. The state of the QFR analysis will be saved on the server, and will be restored when you log on again, from any computer.

To log off from QFR:

- Click Log off 
-  Logging off will NOT cancel an open QFR analysis, you can continue the QFR analysis when you log on to QFR later.
-  Do not leave QFR accessible for unauthorized users. When you leave your workstation, make sure that you log off from QFR and lock the computer system.

14 Description of QFR Results

| | |
|--------------------------------|--|
| Delta QFR: | The pressure drop over a lesion; the change in pressure between the proximal and distal marker. |
| Residual QFR: | A predictive value of the vessel QFR after treatment (revascularization) of a lesion. |
| Vessel QFR: | The flow ratio value for the full length of QFR analysis; the QFR value from the start to the end of the defined target vessel. |
| Lesion length: | The length of the lesion in mm, measured from the proximal lesion marker to the distal lesion marker, in the 3D vessel reconstruction. |
| Minimal Lumen Diameter: | The smallest lumen diameter of the lesion in mm. |
| Reference diameter: | The expected lumen diameter of a healthy vessel at the location of the minimal lumen diameter. |
| Diameter Stenosis %: | The ratio between the diameter reduction and the reference diameter. For example, for a lesion with minimal lumen diameter of 1.0 mm and a reference diameter of 3.0 mm, the diameter reduction is 2.0 mm. The diameter stenosis is $2.0 / 3.0 = 67\%$. |